

Optical Radiation Hazard Analysis

Ultraviolet, Visible and Infrared Optical Sources and Lasers

DAVID H. SLINEY, Ph.D.

Consulting Medical Physicist
406 Streamside Drive
Fallston, MD 21047-2806 USA
Telephone (443) 794-6577
FAX (410) 877-9058

TERRY L. LYON

Consulting Physicist
3 McCann Street
Edgewood, MD 21014-3212 USA
Telephone (410) 612-1270

24 August 2015

Optical Radiation Safety Study Wildfire VioStorm™ UV-LED VS-60 Projection System

INTRODUCTION

Wildfire has developed the VioStorm™ UV-LED VS-60 projection system, which has six 365-nm UV LED emitters (10-W electrical input each) that requires 60-W electrical-input power. This “black light” LED fixture is designed to be on par with current high performance long throw UV-A theater spotlights, which currently employ filtered arc-discharge lamps. The VioStorm incorporates Wildfire's Trias™ digital intuitive three-button monitoring and control system. The VioStorm is a professional product built for professional use and would not be for consumer use. Each LED emitter has optically clear molded silicone optics that resists degradation or yellowing when exposed to high levels of UV. The VioStorm also offers a unique interchangeable optic system that enables the user to configure beam angles to whatever is required for specific applications. The beam can be dimmed by pulse-interval modulation to provide “flicker-free,” 16-bit dimming resolution. The unit can be mounted on the floor or on rails and other environments by a fully adjustable, three-position mounting yoke, which includes an integrated floor stand. A high quality truss clamp and safety cable is also supplied with every fixture. User servicing is accomplished by simply removing the top cover and all components become easily accessible. The VioStorm is a professional UV LED black light fixture with the versatility of a long throw. The VioStorm Series also have four preprogrammed variable-speed effects (Strobe 1-60, Flash 1-60, Pules 1-60 and Random Strobe 1-66) that were tested.

RADIOMETRIC MEASUREMENTS

Instrumentation

1. The initial radiometric reference measurements of the UV LED sources were made with a Gentec Radiometer, Model Ultra UP Series with a Solo2 readout and detector XLP12-1S-H2-D0. The detector had a circular entrance aperture of 11.3 mm (i.e., an area of 1.0 cm²), to measured irradiance as well as power for large beam sizes, and a spectral range of 190 nm to 11 μm. The manufacturer calibrated the detector on 7 January 2013.
2. International Light Technologies, ILT-950 Spectroradiometer #1007094u1 with W2 receptor, calibrated on 7 January 2015.

e-mail: David.Sliney@att.net

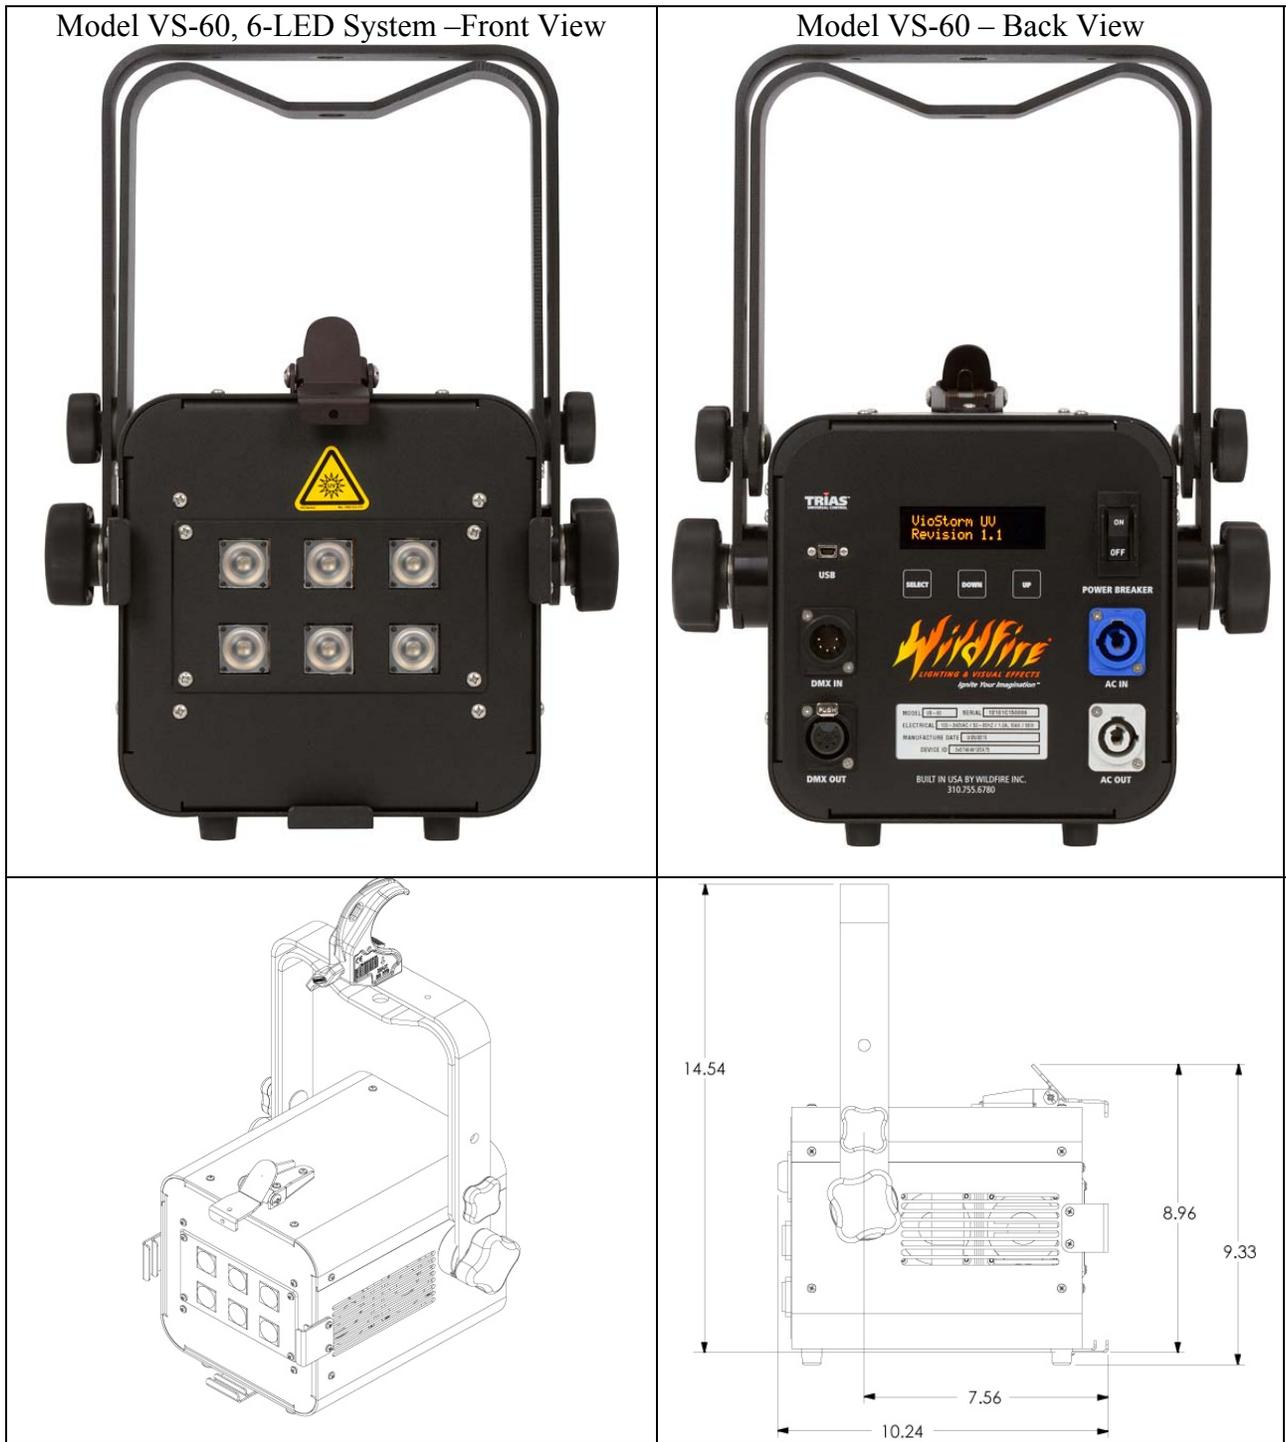


Figure 1. VioStorm UV LED Projection Systems. Top views are photographs of VS-60, six-LED system and bottom panels show line drawings of the VS-60 system (inch dimensions).

3. Recalibrated (using Wildfire LEDs) International Light Technologies, IL1700 readout #1373 with SED038 detector #2200, UVA filter #9322, and window W #5083. Spectral data analysis from the ILT-950 yielded a calibration factor of $6.50 \times 10^{-3} \text{ A} \cdot \text{W}^{-1} \cdot \text{cm}^2$.

4. Oriol ND1 reflecting quartz type filter model 50700 (SN 455) with density of 0.94 at 350 nm and 0.96 at 400 nm. At 368 nm the interpolated transmission for this filter was calculated as 11.3%. Oriol ND3 and ND4 absorbing glass filters models 51000 (SN513) and 51010 (SN248).
5. A Canon G-1 Pro Series digital camera with 2x2 inch filter tray and macro lens set was employed to obtain ultraviolet digital intrabeam images of the source. Oriol ND3 and ND4 absorbing glass filters were employed to reduce the exposure level to the camera image.

Measured Irradiance Values

The VS-60 was measured in the narrow-beam mode to represent the worst-case exposures. The larger, VS-120 model is treated in a separate report. Some very preliminary measurements were: $675 \text{ mW}\cdot\text{cm}^{-2}$ at contact, $96 \text{ mW}\cdot\text{cm}^{-2}$ at 20 cm and $12.5 \text{ mW}\cdot\text{cm}^{-2}$ at 100 cm using the GenTec broad-band thermal radiometer that also responded to infrared radiant energy. However, spectroradiometric measurements (Figure 2) then permitted the determination of total ultraviolet irradiance, as provided in Table 1 below and are plotted later in Figure 3.

Table 1. Unweighted UV irradiance from 300 nm to 400 nm with distance from the front face.

Distance (cm)	VS-60, 6-LEDs ($\text{mW}\cdot\text{cm}^{-2}$)	Single LED package ($\text{mW}\cdot\text{cm}^{-2}$)
1	524	524
5	164	164
10	103.5	52.4
20	65	15.9
40	25.8	4.15
70	9.42	1.55
100	5.14	0.711
150	2.24	0.317
200	1.28	0.194
300	0.596	0.0905
400	0.34	0.0518
500	0.217	0.0340
600	0.157	0.0254

The irradiance data in Table 1 were obtained with an International Light Technologies IL1700 Research Radiometer set with a UV-A receptor that was recalibrated using an ILT950 Spectroradiometer with spectral irradiance data summed from 300 nm to 400 nm. A baffle was employed determine the irradiance of a single LED. Figure 2 shows a typical spectral scan of the ultraviolet source.

Effective UV Irradiance

The actinic UV was also measured and weighted spectrally with the UV hazard function $S(\lambda)$ using a computer spreadsheet. Because stray-light can cause significant errors, spreadsheet analysis was terminated for wavelengths shorter than 310 nm. The effective actinic UV irradiance was determined as $8 \mu\text{W}\cdot\text{cm}^{-2}$ at 20 cm.

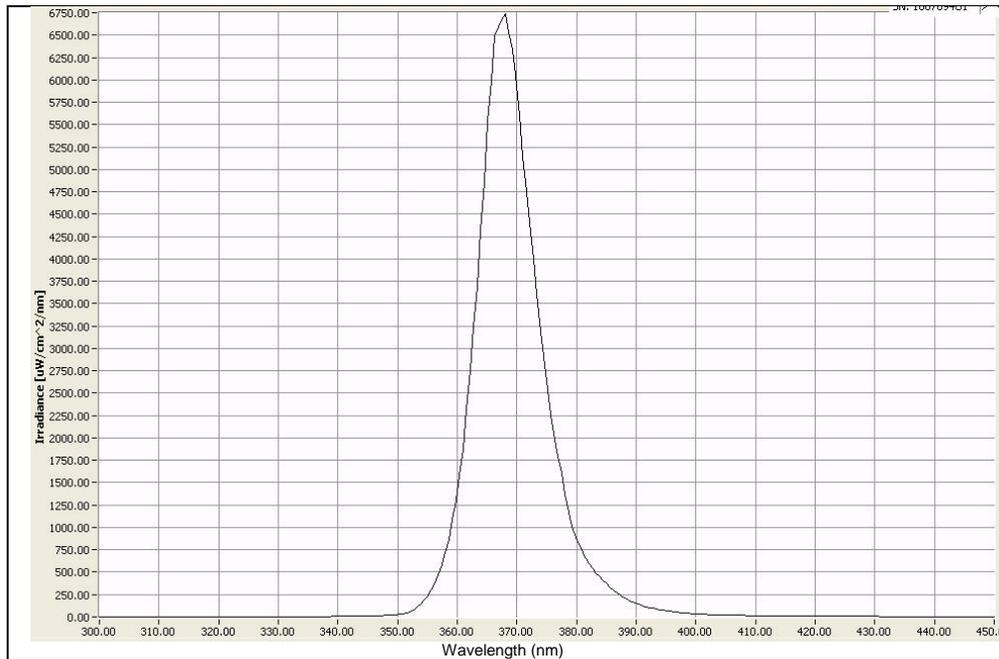


Figure 2. Spectral irradiance at 20 cm from the VS-60, six-LED system. The peak irradiance occurred at ~368 nm with 50% peak-irradiance-points at 362.7 nm and 373.9 nm for a full-width-half-maximum bandwidth of 11.2 nm.

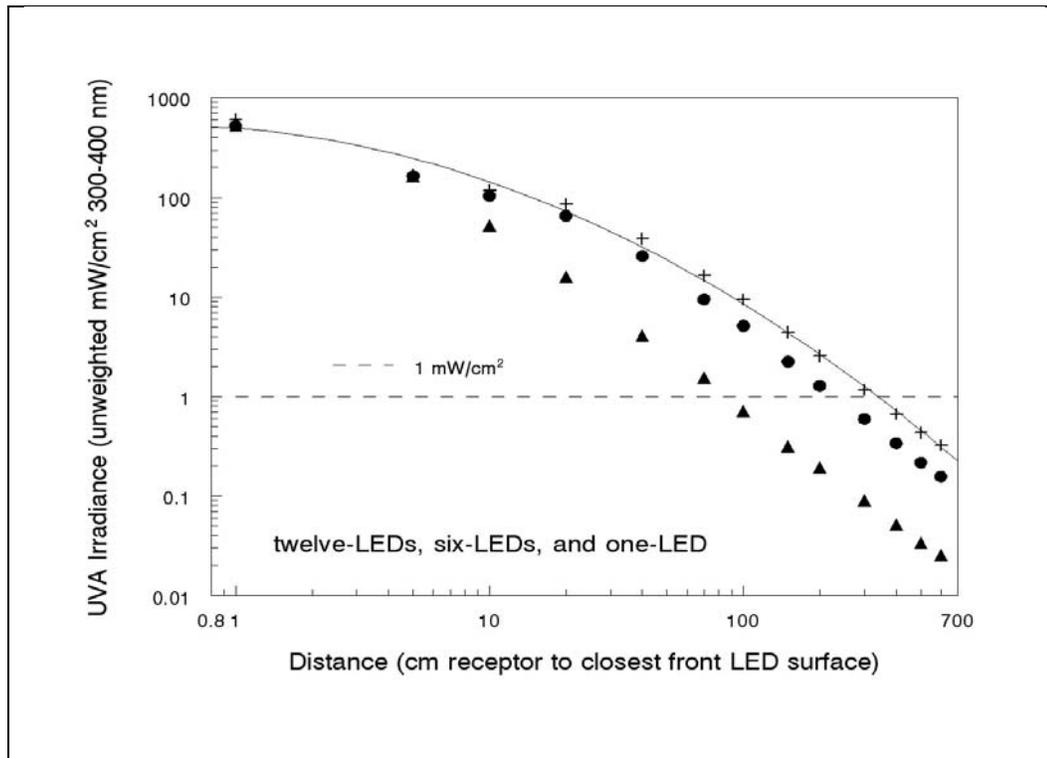


Figure 3. Un-sweighted UVA irradiance from 300 nm to 400 nm with distance from the front face obtained with the ILT-950 spectroradiometer and IL1700 UVA radiometer (●). The top curve (+) is for the higher power, VS-120, 12-LED unit for comparison. The bottom curve is for one-LED (▲). The dashed line is the 1-mW·cm⁻² limit for lengthy ocular exposure.

Radiance Measurements

UV digital imaging and direct radiance measurement were made using the aperture technique. Figure 4 shows the appearance of a single and multiple LED projector elements.

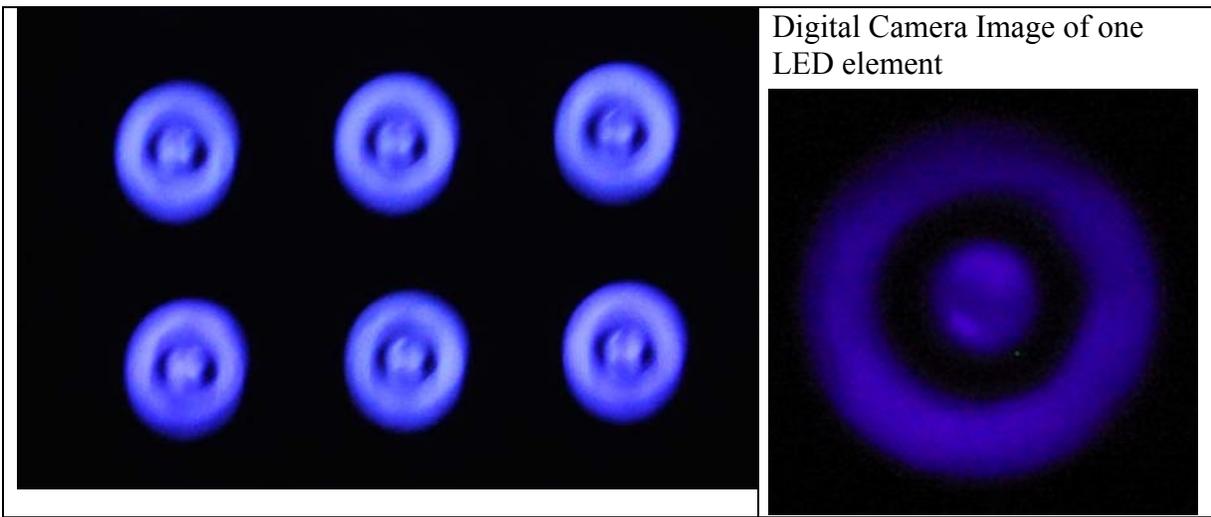


Figure 4. Intra-beam digital photographs of sources operating in the UVA. The left panel shows full array at 40 cm. The right image shows a single LED emitter at 20 cm where each element is not fully flashed. The sources appear indigo-violet in the photo as the camera sensor has very little sensitivity to shorter wavelengths.

The effective blue-light was computed in a spreadsheet as 1.4% of the total irradiance. Using the ILT-950 spectroradiometer at 20 cm with a 2.2 mm aperture placed on the brightest spot of one LED then a spectral weighting spreadsheet was used to determine the effective blue-light radiance as $0.065 \text{ W}\cdot\text{cm}^{-2}\cdot\text{sr}^{-1}$ from 300 nm to 700 nm. The 2.2 mm aperture was scanned across several operating LEDs with a special test fixture employing micrometer adjusters.

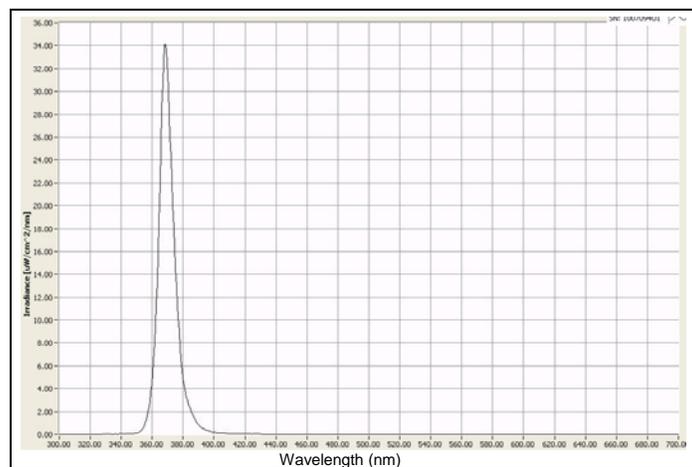


Figure 5. Peak values of spectral radiance from 300 nm to 700 nm observed for an 11 mrad circular aperture (2.2 mm at 20 cm). The spectral irradiance was weighted against the blue-light hazard function and summed then divided by $95 \mu\text{sr}$ to yield an effective blue-light radiance of $0.065 \text{ W}\cdot\text{cm}^{-2}\cdot\text{sr}^{-1}$.

Measurements in the Pulsed Modes

The VS-60 was also operated in several in strobe modes, but all measurements of peak power output indicated that the emissions were little above a gated CW operation. Figure 6 shows an oscilloscope trace with two sets of pulses at intervals of 2.7 ms with large pulses separated from small pulses at ~ 1.3 ms. The large pulses lasted ~ 11.5 μ s and the smaller pulses lasted ~ 12 μ s. In Strobe1, the CW gated pulses lasted ~ 16 ms with 440 ms between repeated pulses. Inside each pulse were 5 large pulses and 6 small pulses. Although the peak pulse power could be slightly above the CW power, but basically the output was almost the same as gated CW. This lead to the conclusion that the hazard assessment was most severe if the device is treated as CW or as gated CW at the same amplitude.

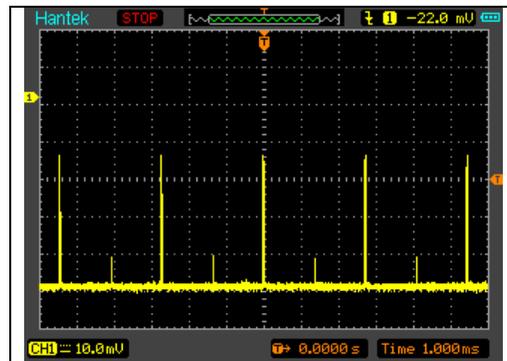


Figure 6. Oscilloscope trace of one of the pulsing modes.

POTENTIAL HAZARDS

The eye is well adapted to protect itself against optical radiation (ultraviolet, visible and infrared radiant energy) from the natural environment and mankind has learned to use protective measures, such as hats and eye-protectors to shield against the harmful effects upon the eye from very intense ultraviolet radiation (UVR) present in sunlight over snow or sand. The eye is also protected against bright light by the natural aversion response to viewing bright light sources. The aversion response normally protects the eye against injury from viewing bright light sources such as the sun, arc lamps and welding arcs, since this aversion limits the duration of exposure to a fraction of a second (about 0.25 s) if substantial visible light is present. Because of the strong fluorescence of the crystalline lens (Zuclich, 2005), some aversion to viewing exists because of the annoyance.

However, the protective benefits of the aversion response are not at play during surgical procedures. There are at least five separate types of hazards to the eye from optical sources, which are recognized and are evaluated for any device (Sloney and Wolbarsht, 1980):

- (a) Ultraviolet photochemical injury to the cornea (photokeratitis) and lens (cataract) of the eye (180 nm to 400 nm). Two exposure limits apply.
- (b) Thermal injury to the retina of the eye (400 nm to 1400 nm).

- (c) Blue-light photochemical injury to the retina of the eye (principally 400 nm to 550 nm; unless aphakic, 310 to 550 nm).
- (d) Near-infrared thermal hazards to the lens (approximately 800 nm to 3000 nm).
- (e) Thermal injury (burns) of the cornea of the eye (approximately 1400 nm to 1 mm).

For the 360-370 nm ultraviolet UV-A LEDs used in the Wildfire projector, only aspect (a) is clearly relevant, and perhaps aspect (c) although little UV-A reaches the retina. And since thermal retinal injury requires much higher radiances, aspect (b) is not possible from LEDs. Aspects (d) and (e) apply only to infrared sources and are therefore not of concern. However, potential thermal hazards to the skin, which normally requires irradiances in the hundreds-of-milliwatts-to-watt range, require analysis. Therefore, this report focuses on the potential *photochemical* effects at the cornea and lens from UV-A. Although the ultraviolet LEDs emit very little energy in the visible and would not be expected to approach limits to protect the eye against aspect (c), these emissions will be analyzed.

UV RADIATION EXPOSURE LIMITS

Ultraviolet radiation exposure criteria have evolved over the last several decades based upon biomedical laboratory research, human epidemiological studies, and clinical experience. These human exposure criteria are presented in regulations, standards and guidelines for product safety and for occupational health. Government agencies issues regulations based on enabling laws passed by legislative bodies. Local, national, or international standardization bodies issue standards. Standards may be developed either through a consensus process, where virtual unanimity exists, or they may be based only on a majority opinion. Guidelines are generally prepared by professional societies as recommendations based upon scientific and medical knowledge. The current UV guidelines are nearly identical internationally for exposure durations less than 1000 seconds.

A number of national and international groups have recommended occupational or public exposure limits (ELs) for UVR. The ultraviolet guidelines of the International Commission for Non-Ionizing Radiation Protection (ICNIRP, 2004) and the American Conference of Governmental Hygienists (ACGIH, 2015) are by far the widest known. Both groups have recommended essentially the same limit based in large part on ocular injury data from animal studies and human accidental injury studies. The primary guideline to protect the skin and the eye is an $S(\lambda)$ weighted daily (8-hour) exposure H_{eff} of $3 \text{ mJ}\cdot\text{cm}^{-2}$ or $30 \text{ J}\cdot\text{m}^{-2}$ referenced to 270 nm, which corresponds to $27 \text{ J}\cdot\text{cm}^{-2}$ at 365 nm. In addition to the primary $S(\lambda)$ -weighted limit, a second limit that is not spectrally weighted is provided to protect the lens from excessive exposure to the UV-A: it is a $1 \text{ J}\cdot\text{cm}^{-2}$ limit applying to all radiant energy between 315 and 400 nm. ACGIH applies this only to exposures less than 1,000 seconds, and recommends a dose-rate limit of $1 \text{ mW}\cdot\text{cm}^{-2}$ for longer exposures. However, ICNIRP applies the $1 \text{ J}\cdot\text{cm}^{-2}$ limit to a full-day (30,000 s) exposure. It is the latter limit that is most restrictive for 360-370 nm. This is a limit that considers chronic outdoor solar exposure over a lifetime, and appears excessively conservative to apply in the context of the relatively brief exposures to the direct beam of the UV-A projector. To place the exposure in perspective, it is useful to consider environmental exposure to the UV in sunlight (Sloney, 2004).

APPLYING THE ICNIRP/ACGIH LIMITS

Ultraviolet Exposure Limits

Two limits apply—a spectrally weighted limit to protect the cornea [Eqn. 1] and an un-weighted UV-A limit [Eqn. 2] :

$$E_{UV} \cdot t = \Sigma E_{\lambda} \cdot S(\lambda) \cdot t \cdot \Delta\lambda = 3 \text{ mJ} \cdot \text{cm}^{-2} \text{ effective (i. e., 28,000 mJ} \cdot \text{cm}^{-2} \text{ at 368 nm)} \quad [1]$$

Which applies to any duration up to one full day; and, to protect the lens and retina:

$$H_{UV-A} < 1.0 \text{ J} \cdot \text{cm}^{-2} \quad \text{for } t < 1,000 \text{ s} \quad [2a]$$

and:

$$E_{UV-A} < 1.0 \text{ mW} \cdot \text{cm}^{-2} \quad \text{for } t > 1,000 \text{ s} \quad [2b]$$

To calculate the maximum direct viewing duration when either [1] or [2] is not satisfied, the maximum "stare time," t_{\max} , is found by inverting Eqn. [1] or [2a] for a CW source with a weighted or un-weighted irradiance.

$$t_{\max} = 3 \text{ mJ} \cdot \text{cm}^{-2} / E_{UV} \quad \text{for the } S(\lambda)\text{-weighted value} \quad [3a]$$

$$t_{\max} = 1.0 \text{ J} \cdot \text{cm}^{-2} / E_{UV-A} \quad \text{for the UV-A} \quad [3b]$$

For example, at a distance of 1 m, the total irradiance from the VS 60 was $5.14 \text{ mW} \cdot \text{cm}^{-2}$, hence the t_{\max} from Eqn. [3b] would be: $1.0 \text{ J} \cdot \text{cm}^{-2} / (0.00514 \text{ W} \cdot \text{cm}^{-2}) = 195 \text{ s}$. And at only 20 cm, because a small amount of UV-B (280 – 315 nm) radiation was measured, the effective irradiance from [3a] was $8 \mu\text{W} \cdot \text{cm}^{-2}$ at 20 cm, and the permissible exposure duration t_{\max} would be 375 s. Hence the limiting case will be the limit of [3b]. Indeed, the permissible exposure duration at 20 cm from [3b] would be only $(1.0 \text{ J} \cdot \text{cm}^{-2}) / (0.065 \text{ W} \cdot \text{cm}^{-2}) = 15.4 \text{ s}$. At that irradiance the temperature rise in the skin would limit the exposure faster.

Blue-Light Photochemical Retinal Hazard

The ACGIH TLV (ACGIH, 2010) and ICNIRP guidelines (ICNIRP, 2004) are identical for large sources and are designed to protect the human retina against photoreinitis, "the blue-light hazard" is an effective blue-light radiance L_B spectrally weighted against the Blue-Light Hazard action spectrum $B(\lambda)$ and integrated for t s of $100 \text{ J} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1}$, for $t < 10,000 \text{ s}$, i.e.,

$$L_B \cdot t = \Sigma L_{\lambda} \cdot B(\lambda) \cdot t \cdot \Delta\lambda \leq 100 \text{ J} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1} \text{ effective} \quad [4]$$

and for $t > 10,000 \text{ s}$ (2.8 hrs.):

$$L_B \leq 10 \text{ mW} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1} \quad \text{for } t > 10,000 \text{ s} \quad [5]$$

To calculate the maximum direct viewing duration when [5] is not satisfied, this maximum "stare time," t_{\max} , is found by inverting Eqn. [4] for a CW source with a weighted radiance of L_B :

$$t_{\max} = (100 \text{ J} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1}) / L_B \quad [6]$$

The radiance values are averaged over a field of view which is not less than $11 \text{ mrad} = 0.011 \text{ rad}$. The blue light hazard is evaluated by mathematically weighting the spectral irradiance, E_λ , against the blue-light hazard function to obtain E_B ; however, because the 370 nm radiation is largely absorbed at the lens, less than 1% reaches the retina, and the spectral weighting function value of $B(\lambda)$ is 0.01. Hence the limit would be $1.0 \text{ W} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1}$ for $t > 10,000 \text{ s}$, which was exceeded by the maximum radiance of the source. The measured effective blue-light radiance was $0.065 \text{ W} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1}$ from 300 nm to 700 nm as measured at 20 cm. Although unlikely, an accidental exposure at a 20-cm viewing distance would only be momentary. The duration t_{\max} for staring at the source can be calculated from Eqn. [6], and would be $L_A = (100 \text{ J} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1}) / (0.065 \text{ W} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1}) = 1540 \text{ s} = 25.6 \text{ minutes}$. This long stare time - which is not reasonably foreseeable because of glare and lens fluorescence - would be for the normal (phakic) eye. Certainly the maximal worst-case exposure to the operator from reflections from many hours of operation a day could not exceed any of the applicable limits. However, in the very rare instance of an aphakic person (no crystalline lens) viewing the direct source, the weighting factor shifts from $B(\lambda)$ to $A(\lambda)$ and the spectral weighting factor for 368 nm becomes 4.0 and the effective aphakic radiance L_A becomes: $4.0(6.5 \text{ W} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1}) = 26 \text{ W} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1}$. This means that the stare-time would be reduced to only $\sim 4 \text{ s}$. However, an aphakic person would see a very strongly bright source, and the actual exposure would be reduced to the standardized 0.25 s aversion response to bright light.

The above exposure guidelines apply to the awake, task-oriented eye and incorporate an underlying assumption that the eye's pupil constricts with bright light, that the aversion response limits exposure duration, and that eye-movements are not restricted.

HAZARD ANALYSIS

The VS-60 emits irradiance values well in excess of lengthy UV-A exposure limits; however, the units can be safely used - as their arc-lamp predecessors - by properly mounting the units away from accessible occupied areas for the first 2.5 m (see Table 1) of the throw to remain below the continuous UV exposure limit of $1 \text{ mW} \cdot \text{cm}^{-2}$.

Assessment Distance and Risk Group

ANSI/IESNA RP27.3 specifies a measurement distance of 20 cm for bare lamps, but with an assessment distance where the illuminance reaches 500 lx for general light service (GLS) lamps. However, no assessment distance was provided for some specialized applications such as searchlights or UV spotlights. Assessment distances were not provided for other types of non-GLS lamp products, although this was intended to be provided in vertical (application-specific) standards. IEC standard 62471 follows the ANSI/IESNA RP27.3 emission limits and the default measurement distance of 20 cm; however, IEC 62471-5 is a vertical standard for image projectors, and specifies an assessment distance of 1 m. Some suggested assessment distances for searchlights have been 2-3 m or even greater distances. But, using a very conservative, 1-m assessment distance, the irradiance of the VS-60 is $5.1 \text{ mW} \cdot \text{cm}^{-2}$, which places it clearly into Risk Group RG-2. The RG-2 Emission Limit is $E_{UV} = 3 \mu\text{W} \cdot \text{cm}^{-2}$ for Actinic UV effective irradiance, and $400 \text{ W} \cdot \text{cm}^{-2} \cdot \text{sr}^{-1}$ for L_B . The measured actinic E_{UV} at 20 cm was $8 \mu\text{W} \cdot \text{cm}^{-2}$, which if extrapolated to 100 cm would be less than $1.0 \mu\text{W} \cdot \text{cm}^{-2}$, which is well below the limit of

$3 \mu\text{W}\cdot\text{cm}^{-2}$ for RG-2. Continuous exposure for many hours at 100 cm is not assumed to be reasonably foreseeable for RG-2 products. Actually, a more realistic assessment distance for a professional theatrical spotlight or specialty projection system like the VS-60, is more likely to be set at no less than 200 cm, where the irradiance falls to $\sim 1.3 \text{ mW}\cdot\text{cm}^{-2}$; which is below the $3.3\text{-mW}\cdot\text{cm}^{-2}$ RG-1 (very low risk) category for UV-A. A caution distance (sometimes referred to as a “hazard distance,” even if not RG-3) exists to a distance of 1.3 m (130 cm \sim 4.3 feet) where the beam irradiance falls below $3.3 \text{ mW}\cdot\text{cm}^{-2}$. Finally, the distance to $1 \text{ mW}\cdot\text{cm}^{-2}$ for continuous staring into the beam would be 3.3 m, or 11 feet.

CONCLUSION AND RECOMMENDATIONS

The VSS-60 poses no significant hazard beyond 1 meter, and momentary exposures within that distance are not hazardous. However, persons should be warned not to stand in the beam within 1 meter, and not to continuously stare directly into the source within 1.3 m (4.3 feet). A warning label should so indicate



Terry L. Lyon



David H. Sliney, Ph.D.

REFERENCES

1. American Conference of Governmental Industrial Hygienists (ACGIH), *2015 TLV's, Threshold Limit Values for Chemical Substances and Physical Agents & Biological Exposure Indices*, Cincinnati: ACGIH.
2. American Conference of Governmental Industrial Hygienists (ACGIH), *Documentation of the Threshold Limit Values for Physical Agents*, 7th Edn. (2001), with 2002-2015 supplements, ACGIH Publication #0100DocP/A, Cincinnati: ACGIH (2015).
3. International Commission on Non-Ionizing Radiation Protection (ICNIRP), Guidelines on Limits of Exposure to Ultraviolet Radiation of Wavelengths between 180 nm and 400 nm (Incoherent Optical Radiation), *Health Physics* 87(2), 171-186, 2004.
4. World Health Organization (WHO) 1994 *Environmental Health Criteria No. 160, Ultraviolet Radiation*, joint publication of the United Nations Environmental Program, the International Radiation Protection Association and the World Health Organization (Geneva: WHO).
5. Sliney, D.H., and Wolbarsht, M.L., *Safety with Lasers and Other Optical Sources* (New York: Plenum Publishing Corp), 1980.
6. International Electrotechnical Commission (IEC). 60825-1

7. International Commission on Non-Ionizing Radiation Protection (ICNIRP) (2013) ICNIRP guidelines on limits of exposure to incoherent visible and infrared radiation, *Health Phys*, **105**(1):74-91.
8. International Commission on Non-Ionizing Radiation Protection (ICNIRP) (2013) ICNIRP guidelines on limits of exposure to laser radiation of wavelengths between 180 nm and 1,000 μm , *Health Phys.*, **105**(3):271-295.
9. American National Standards Institute/Illuminating Engineering Society of North America (ANSI/IESNA) (2005) *Photobiological Safety of Lamps and Lighting Systems—General Requirements, RP27.1-05*, New York, IESNA.
10. American National Standards Institute/Illuminating Engineering Society of North America (ANSI/IESNA) (2000) *Photobiological Safety of Lamps and Lighting System—Measurement Systems - Techniques, RP27.2-00*, New York, IESNA.
11. American National Standards Institute/Illuminating Engineering Society of North America (ANSI/IESNA) (2007) *Photobiological Safety of Lamps and Lighting Systems—Risk Group Classification and Labeling, RP27.3-07*, New York, IESNA.
12. CIE (Commission International de l’Eclairage, the International Commission on Illumination) (2002) CIE Standard S-009E-2002, *Photobiological Safety of Lamps and Lamp Systems*, Vienna, CIE. **Adopted as a joint-logo standard by the International Electrotechnical Commission (IEC) in 2006, as IEC 62471/CIES009-2006.**
13. International Standards Organization (ISO), (2007), International Standard, ISO 15004-2:2007, *Ophthalmic Instruments—Fundamental requirements and test methods—Part 2: Light hazard protection*, Geneva, ISO.
14. Ham WT Jr, Mueller HA, Ruffolo JJ Jr, Guerry D III, Guerry RK., Action spectrum for retinal injury from near-ultraviolet radiation in the aphakic monkey. *Am J Ophthalmol*; 93:299–306 (1982).
15. Sliney DH, Estimating the solar ultraviolet radiation exposure to an intraocular lens implant, *J Cataract Refract Surg*, **13**(5):296-301, 1987.
16. Zuclich, J.A., Ultraviolet-induced photochemical damage in ocular tissues, *Health Physics* 56(5), 671-682 (1989).